




SETTING UP A PCR LAB

By

Prof. Dr. Asmaa A. A. Hussein
Prof. of Zoonoses & Director of the
MBRU

Assiut University




PCR lab should consist of **3** distinct work areas


In order to avoid the **contamination problems**, each area should be dedicated to a single procedure

First area → **Specimen preparation**

Second area → **Reagent preparation & PCR set-up**

Third area → **Amplification & detection**



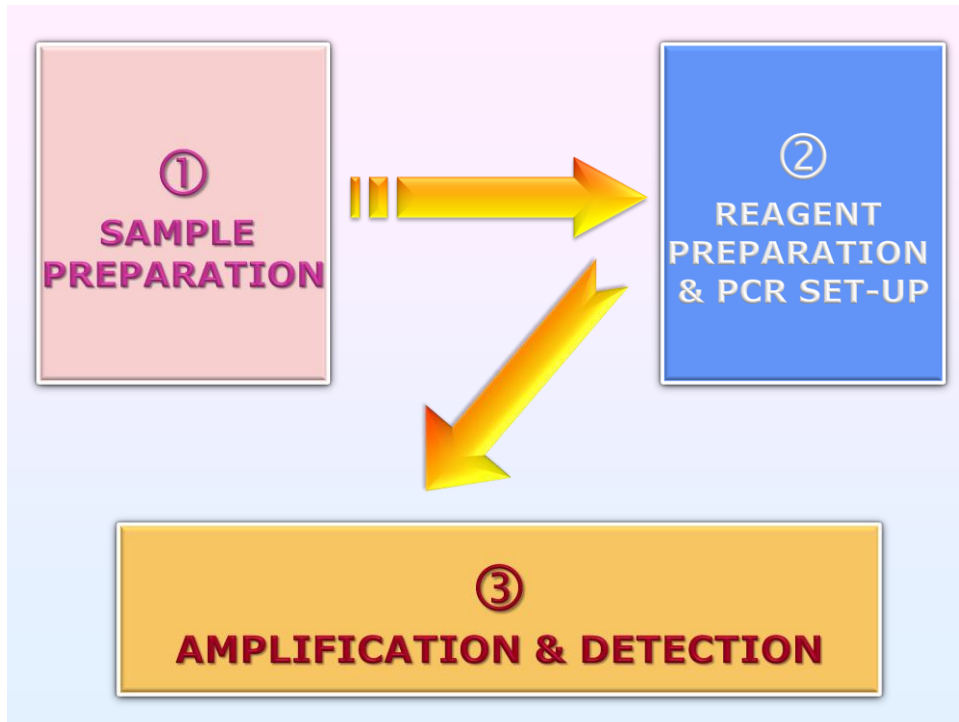


AREA 1: SAMPLE PREPARATION:


- ✱ **Positive-displacement pipettes or pipettors with aerosol-resistant tips**
- ✱ **Gloves & laboratory coat**
- ✱ **Refrigerator, freezer, water bath or dry - heat block, laminar flow biosafety cabinet**
- ✱ **Cell lysis reagents**



AREA 2: REAGENT PREPARATION & PCR SET-UP:

- **Amplification reagents & supplies**
 - **Positive-displacement pipettes or pipettors with aerosol-resistant tips**
 - **Laminar-flow biosafety cabinet or dead air box**
 - **Gloves & laboratory coat**
 - **Refrigerator & freezer**
 - **Water bath or dry – heat block**
- 


AREA 3: AMPLIFICATION & DETECTION:

- ☑ **Thermal cycler**
 - ☑ **Pipettors with aerosol-resistant tips**
 - ☑ **Detection equipment (electrophoresis unit, incubator, plate washer, plate reader, water bath)**
 - ☑ **Refrigerator & freezer**
 - ☑ **Reagents & supplies for detection**
- 

The following practices will diminish the potential for contamination:

- ★ **Each area should have dedicated supplies & reagents**
- ★ **Color coding of reagents & supplies identifies those that belong to a particular area**
- ★ **Reagents, supplies & equipment should never be taken from one area to another, three sets of pipettors are essential**

- ★ **The workflow must be unidirectional from “clean” (pre-PCR) to “dirty” (post-PCR)**
- ★ **Dedicated labcoats & gloves should be worn at each work site**
- ★ **When moving to a new area, workers should put on new gloves & labcoats**





PCR LABORATORY ORGANIZATION

Flow of samples
for PCR analysis

PRE-PCR LAB → POST-PCR LAB

Pre-PCR is the protocols & equipment required for the isolation of nucleic acid & assembly of the reaction to amplify the samples

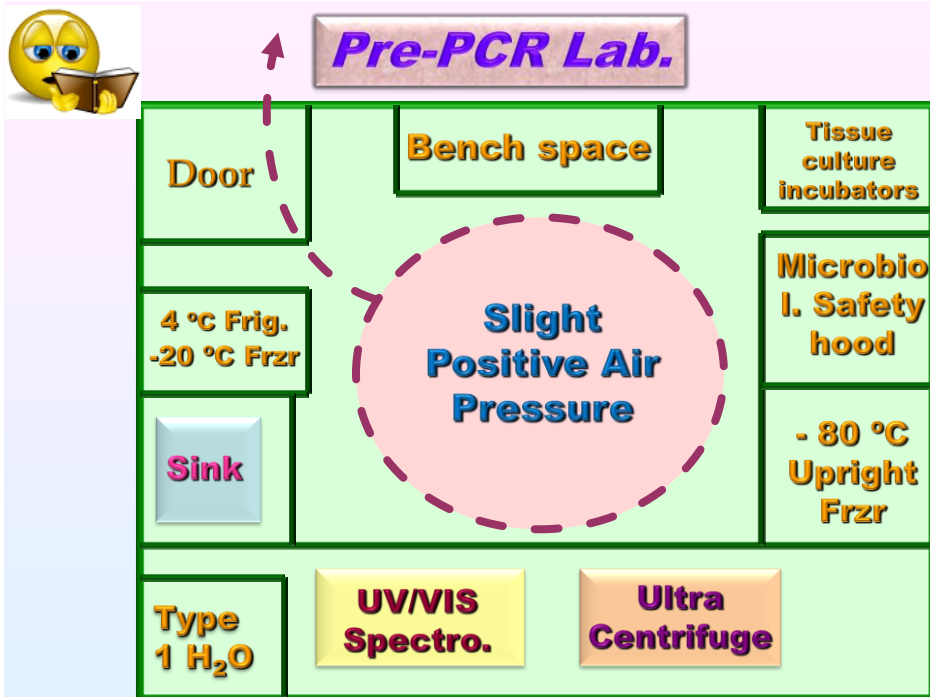

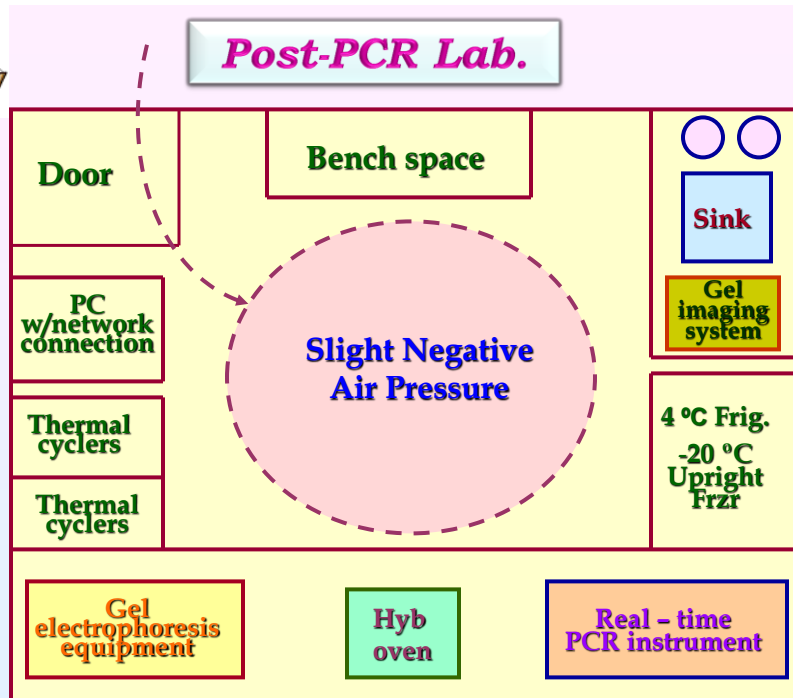

Centrifuge



Avanti Centrifuge



Optical Microscopes



Safety Cabinet



Gel tank (to place the gel mold and run electrophoresis)




Gel documentation (capture and print the image of agarose gel)




UV transilluminator (basic device for visualizing fluorescence-stained gels)




Example of an image captured by gel documentation and UV transilluminator of the gel agarose electrophoresis

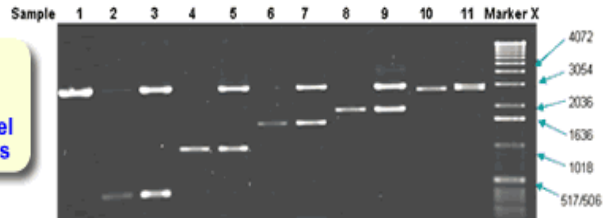

Thermal Cycler

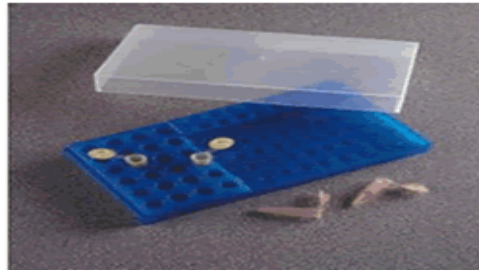

PCR microcentrifuge tubes (0.5µl)

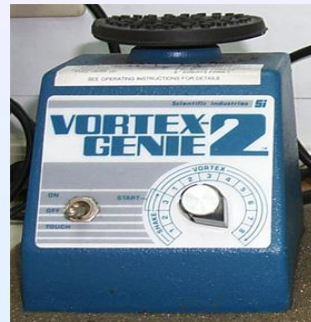





Strict adherence to proper laboratory technique:

- **Physically isolate PCR preparations & products**
- **Autoclave solution**
- **Aliquot reagents**
- **Use disposable gloves & change gloves often during set-up**
- **Avoid splashes**

- **Use positive-displacement pipettes or aerosol resistant tips on air-displacement pipettes**
- **“ Premix” reagents**
- **Add DNA last**
- **Choose positive & negative controls carefully**





*Thank you for your
attention!*

